

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0009
Location:	DUNELLEN POLICE DEPT.	Calib. No.:	00044
Calibration File No.:	01438	Cert. Date:	12/03/2020
Certification File No.:	01439	Lin. Date:	12/03/2020
Linearity File No.:	01440	Soln. Date:	05/07/2021
Solution File No.:	01477	File Date:	05/07/2021
Sequential File No.:	01477		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0213
Solution Control Lot:	20320	Expires:	07/06/2022
		Bottle No.:	0964

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:38D		
Control 1 EC	0.100%	20:39D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	20:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:40D		
Control 2 EC	0.100%	20:41D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	20:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:41D		
Control 3 EC	0.101%	20:42D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	20:42D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:43D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: NIERODZIK

First Name: MARCIN


MI: -

Signature: _____

Marcin Nierodzik #46

Badge No.: 46

Date: 05/07/2021

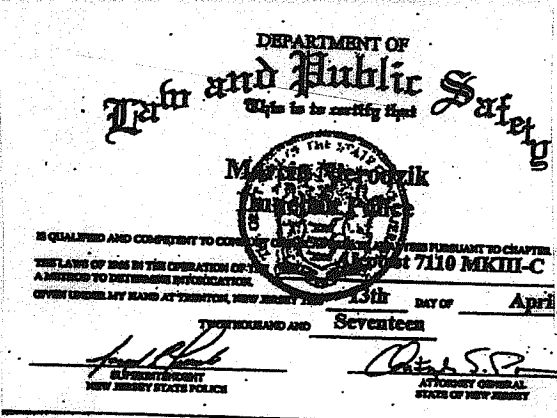

Certificate of Training		
This is to certify that		
Marcin Nierodzik		
has successfully completed practitioner training in the use of		
Horizontal Gaze Nystagmus		
Improved Sobriety Test Procedures		
as set forth by the National Highway Traffic Safety Administration		
		Instructor
ORIGINAL COURSE DATES		
DATE	Refresher Course PLACE	INSTRUCTOR
1. 12/14/15	Sayreville PD	Cham
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____