

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0009
Location: DUNELLEN POLICE DEPT.
Calibration File No.: 01529 Calib. Date: 03/15/2022 Calib. No.: 00047
Certification File No.: 01530 Cert. Date: 03/15/2022 Cert. No.: 00038
Linearity File No.: 01531 Lin. Date: 03/15/2022 Lin. No.: 00039
Solution File No.: 01537 Soln. Date: 04/14/2022 Soln. No.: 00293
Sequential File No.: 01537 File Date: 04/14/2022

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0218
Control Solution %: 0.100% Expires: 03/17/2023
Solution Control Lot: 21090 Bottle No.: 0951

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:13D		
Control 1 EC	0.098%	20:14D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:15D		
Control 2 EC	0.098%	20:15D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:16D		
Control 3 EC	0.098%	20:17D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:18D		

All tests within acceptable tolerance.

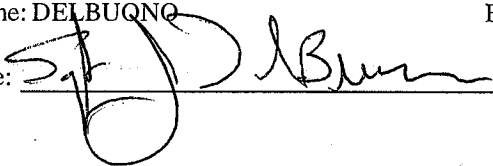
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELBUONO

First Name: JEFFREY

MI: M

Signature: 

Badge No.: 32

Date: 04/14/2022