

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0009
Location: DUNELLEN POLICE DEPT.
Calibration File No.: 01303 **Calib. Date:** 05/20/2019 **Calib. No.:** 00040
Certification File No.: 01304 **Cert. Date:** 05/20/2019 **Cert. No.:** 00031
Linearity File No.: 01305 **Lin. Date:** 05/20/2019 **Lin. No.:** 00032
Solution File No.: 01314 **Soln. Date:** 06/21/2019 **Soln. No.:** 00256
Sequential File No.: 01314 **File Date:** 06/21/2019

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0218
Control Solution %: 0.100% **Expires:** 09/17/2020
Solution Control Lot: 18290 **Bottle No.:** 1255

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:35D		
Control 1 EC	0.101%	23:35D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	23:35D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:36D		
Control 2 EC	0.100%	23:37D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	23:37D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:37D		
Control 3 EC	0.100%	23:38D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	23:38D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:39D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DELBUONO


First Name: JEFFREY

MI: M

Signature: 

Badge No.: 32

Date: 06/21/2019

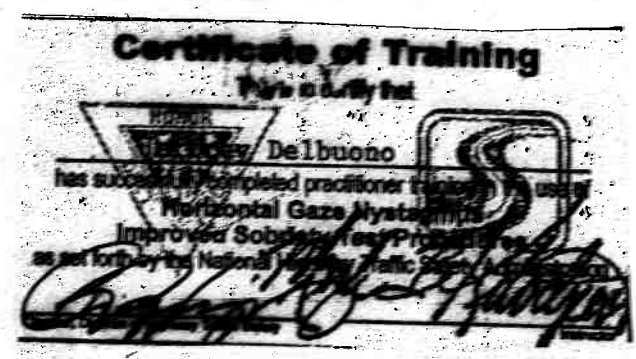

ORIGINAL COURSE DATES

DATE	PLACE	INSTRUCTOR
2-24-11	SAYREVILLE PD	
5-7-13	SAYREVILLE	
1-13-15	SAYREVILLE PD	
7/6/17	SAYREVILLE PD	R.D. 7